

# Experience share on veterinary drug multi-residue analysis

www.amarc.co.th



Nittaya Tangpakdeerat  
Bangkok, Thailand  
E-mail : Nittayatang@gmail.com





# Outline

1

**Introduction**

2

**Applied methods of analysis**

3

**Technical Comments**



# Introduction

PT sample

Sample A



- 1) 3-amino-2-oxazolidone (AOZ)
- 2) 5-morpholinomethyl-3-amino-2-oxazolidone (AMOZ)
- 3) Sulfamethoxazole
- 4) Sulfadimidine
- 5) Sulfaquinoxaline
- 6) Ciprofloxacin

Sample B



Freeze dried chicken contained in sealed foil bag




# Introduction

## Nitrofurans

Parent drug  
unstable

Mild acid in human

Metabolites form

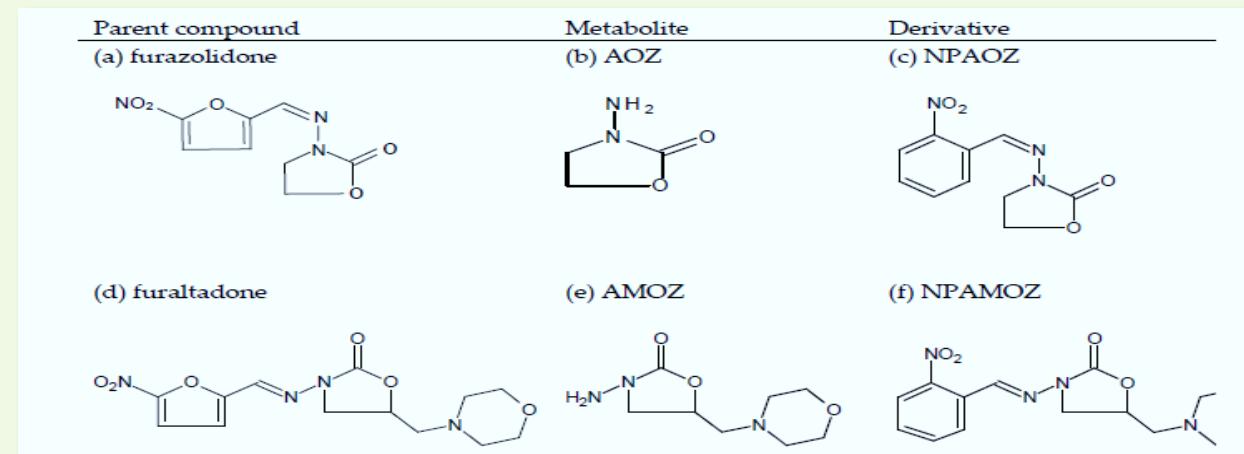

- Broad spectrum synthetic antimicrobial agents
- used to prevent gastrointestinal infections
- mutagenic and carcinogenic



# Introduction

## The Minimum Required Performance Limits (MRPL)


Compound	(µg/kg)
Nitrofurans Metabolites (SEM, AOZ, AMOZ, AHD)	1

Ref : Commission Decision 2003/181/EC.



# Introduction

Ciprofloxacin is amphoteric compound that is soluble in polar organic solvents, slightly soluble in water and insoluble nonpolar solvents

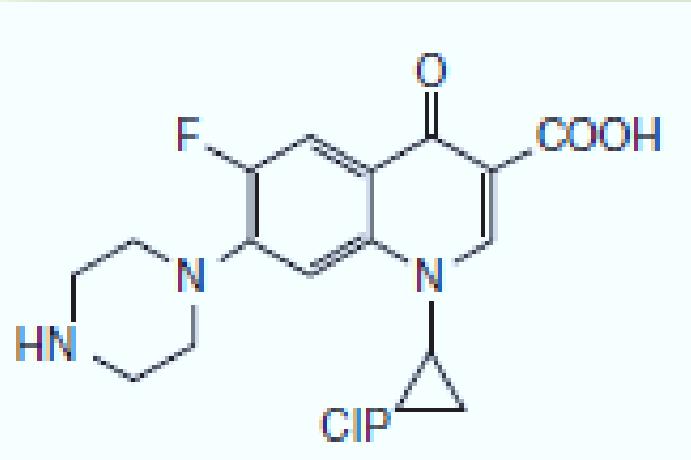

Nikolaos A. Botsoglou, *Encyclopedia of Chromatography*



# Introduction

## The maximum residue limits (MRL)


Compound	in muscle ( $\mu\text{g/kg}$ )
Sum of Enrofloxacin and Ciprofloxacin	100

Ref : Commission Regulation (EU) 37/2010 of 22 December 2009 on pharmacologically active substances and their classification regarding maximum residue limits in foodstuffs of animal origin, OJ L 15/1, 20.01.2010, p. 29 (ANNEX I).




# Introduction


Sulfonamides are one class of antimicrobial agent used widely in the livestock industry to promote growth

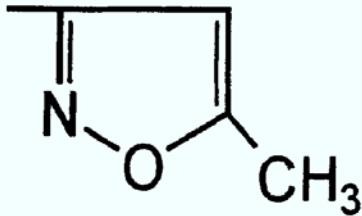

sulphamethoxazole



sulphadimidine

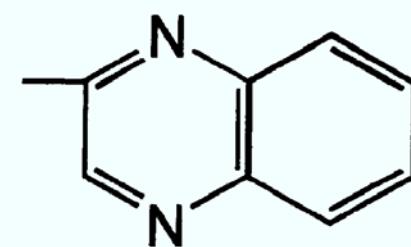

sulphaquinoxaline



# Introduction

## The maximum residue limits (MRL)


Compound	in muscle ( $\mu\text{g/kg}$ )
Sulfonamides (all substances belonging to the sulfonamide group)	100

Ref : Commission Regulation (EU) 37/2010 of 22 December 2009 on pharmacologically active substances and their classification regarding maximum residue limits in foodstuffs of animal origin, OJ L 15/1, 20.01.2010, p. 1–2 (ANNEX I).



# Applied methods of analysis

## Nitrofurans Metabolite (AOZ, AMOZ)

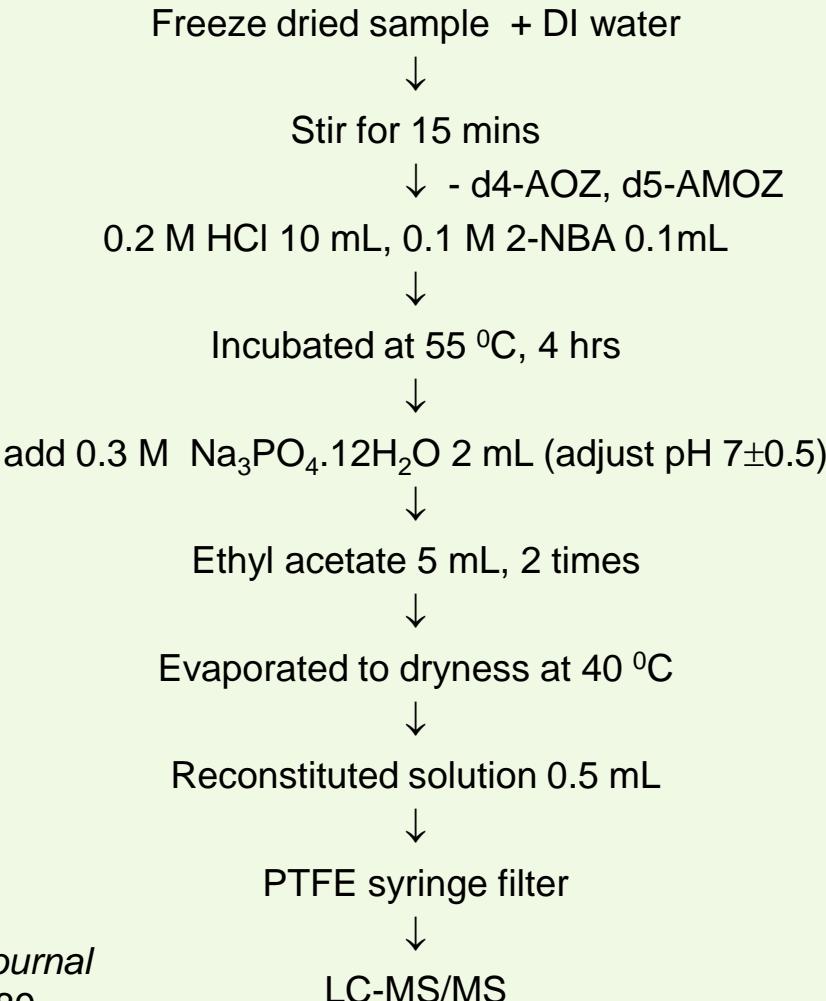



# Applied methods of analysis


## Determination technique

LC-MS/MS	:	Agilent model HP1200, 6410A
Column	:	Symmetry C18, 3.9 mm x 150 mm
Flow rate	:	0.4 mL / min
Run time	:	10 min
Column temperature	:	40 °C
Injection volume	:	10 µL
Mobile phase A	:	0.1 % Formic acid in DI water
Mobile phase B	:	0.1 % Formic acid in Acetonitrile
Ion source	:	ESI
Ion Polarity	:	Positive
Delta EMV	:	600 V
Gas Temp	:	325 °C
Gas Flow	:	10 L/min
Nubulizer	:	50 psi
Capillary	:	4500 V








# Applied methods of analysis

Compound Name	Precursor Ion (m/z)	Product Ion (m/z)	Dwell	Fragmentor (V)	Collision Energy (eV)
AOZ	236	134	30	120	6
	236	104	30	120	22
d4-AOZ	240	134	30	110	4
AMOZ	335	291	30	90	3
	335	262	30	90	12
d5-AMOZ	340	296	30	120	7




# Applied methods of analysis

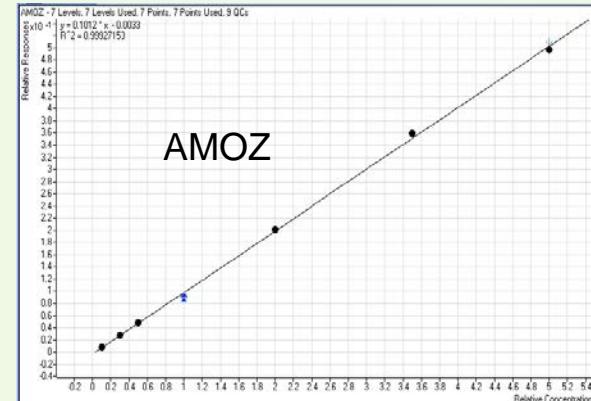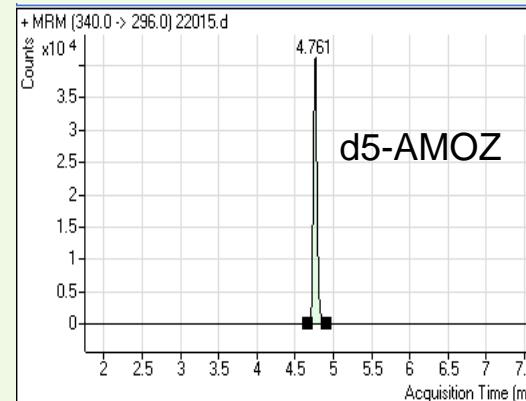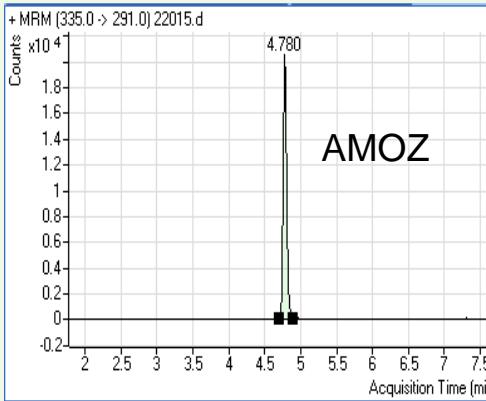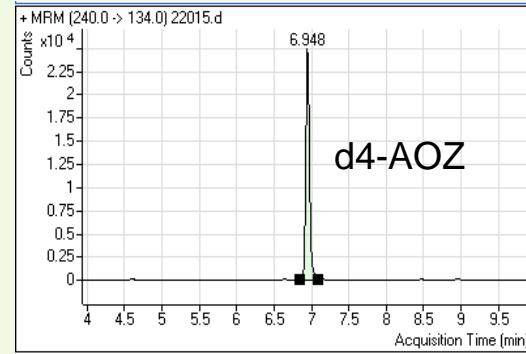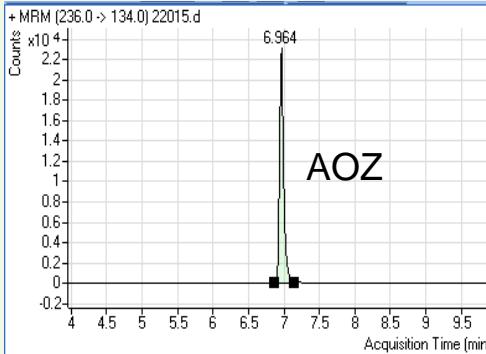



# Applied methods of analysis

- Fluoroquinolone (Ciprofloxacin)

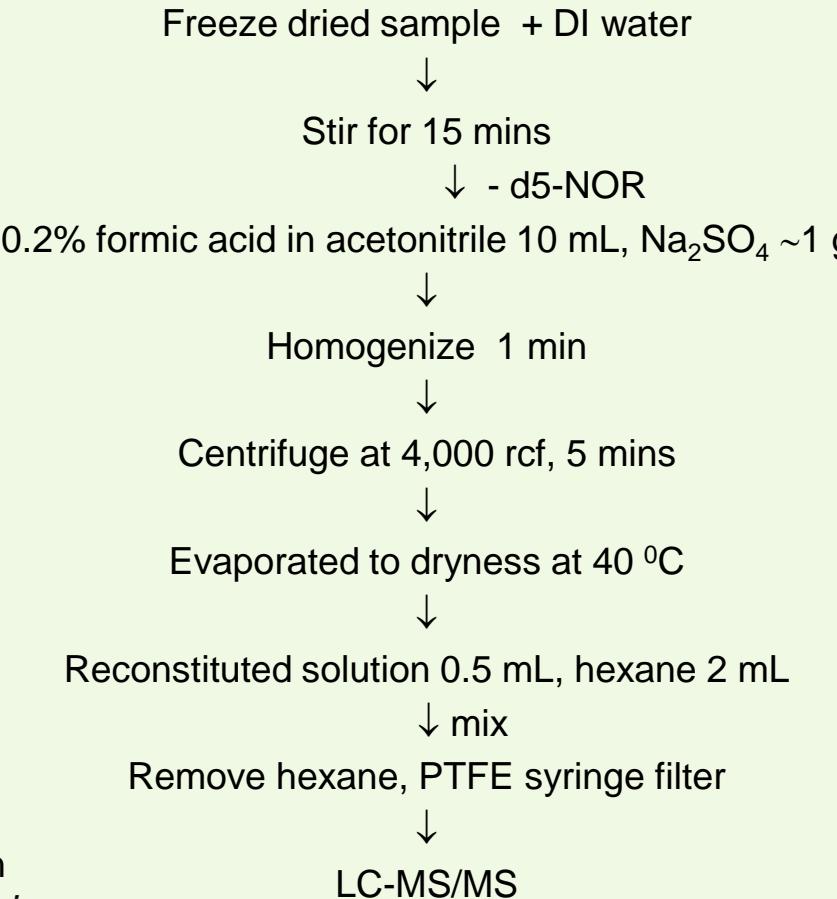

Ref : In - house method based on  
*Journal of Food and Drug Analysis*  
Vol. 18, No.2, 2010, p. 87-97



# Applied methods of analysis

## Determination technique




LC-MS/MS	:	Agilent model HP1200, 6410A
Column	:	Symmetry C18, 3.9 mm x 150 mm
Flow rate	:	0.5 mL / min
Run time	:	7 min
Column temperature	:	35 °C
Injection volume	:	20 µL
Mobile phase A	:	0.1 % Formic acid in DI water
Mobile phase B	:	Acetonitrile
Ion source	:	ESI
Ion Polarity	:	Positive
Delta EMV	:	500 V
Gas Temp	:	325 °C
Gas Flow	:	10 L/min
Nubulizer	:	45 psi
Capillary	:	3500 V



# Applied methods of analysis

Compound Name	Precursor Ion (m/z)	Product Ion (m/z)	Dwell	Fragmentor (V)	Collision Energy (eV)
CIP	332	314	25	100	20
		288	25	100	15
d5-NOR	325	307	25	100	20

(CIP = Ciprofloxacin, d5-NOR = d5-Norfloxacin)

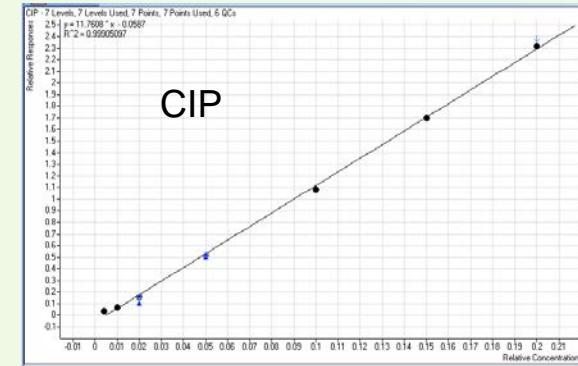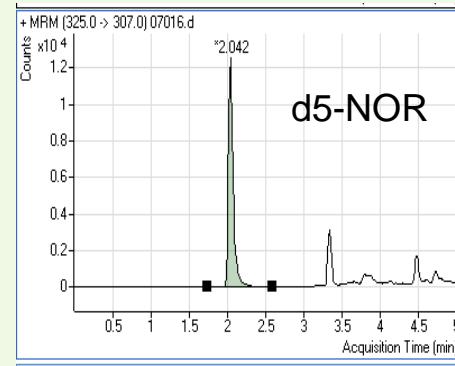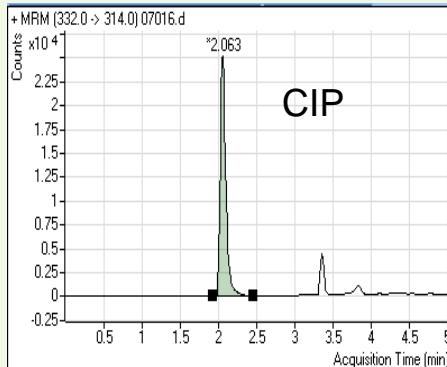



# Applied methods of analysis

## Sulfonamides (Sulfamethoxazole, Sulfadimidine, Sulfaquinoxaline)

Freeze dried sample + DI water  
↓  
Stir for 15 mins  
↓ - d4-SMR  
0.2 M HCl 5 mL, vortex  
↓ Incubate at room temp 30 mins  
0.3 M citric acid 20 mL  
↓ adjust pH ~ 4  
Vortex, centrifuge at 4000 rcf, 5 mins  
↓  
Load SPE cartridge (OASIS HLB 200 mg/6 mL)  
↓ - pre-condition ACN 5 mL, DI water 5 mL  
Load sample  
↓ - wash DI water 5 mL  
Eluted ACN 5 mL, evaporated to dryness at 40 °C  
↓  
Reconstituted solution 1 mL, PTFE syringe filter  
↓  
LC-MS/MS



# Applied methods of analysis

## Determination technique






LC-MS/MS	:	Agilent model HP1200, 6410A
Column	:	Symmetry C18, 3.9 mm x 150 mm
Flow rate	:	0.5 mL / min
Run time	:	7 min
Column temperature	:	35 °C
Injection volume	:	10 µL
Mobile phase A	:	0.1 % Formic acid
Mobile phase B	:	0.1 % Formic acid in acetonitrile
Ion source	:	ESI
Ion Polarity	:	Positive
Delta EMV	:	600 V
Gas Temp	:	325 °C
Gas Flow	:	10 L/min
Nubulizer	:	35 psi
Capillary	:	5000 V



# Applied methods of analysis

Compound Name	Precursor Ion (m/z)	Product Ion (m/z)	Dwell	Fragmentor (V)	Collision Energy (eV)
SMX	254.2	156	15	100	10
	254.2	188	15	100	10
SDD	279.2	186	15	100	20
	279.2	156	15	100	20
SQX	301	156	15	130	10
	301	146	15	130	10
d4-SMR	265.2	109.9	15	100	10

(SMX = Sulfamethoxazole, SDD = Sulfadimidine, SQX = Sulfaquinoxaline, d4-SMR = d4- sulfamerazine)

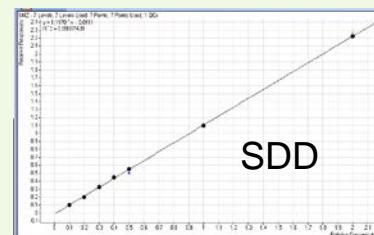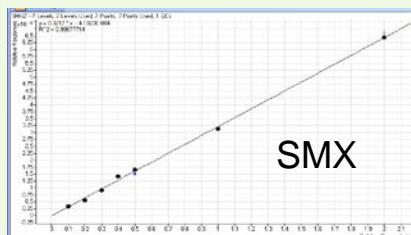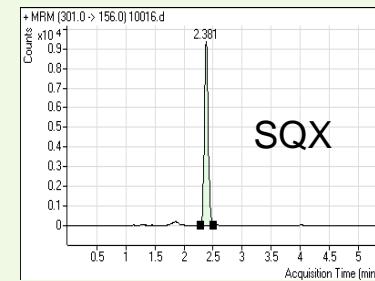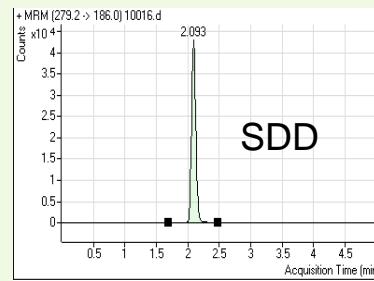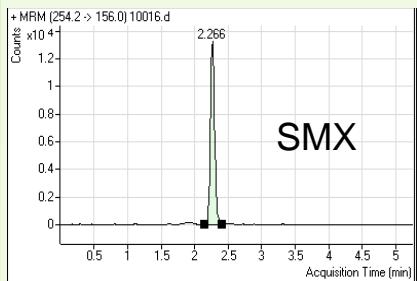



# Technical Comments

## Factor affecting the test

- Moisture
- pH
- Time
- Temperature





# Technical Comments

- Sample handling error
- Inadequate methods
- Equipment failure
- Calculation error
- Reporting error



# Technical Comments

- Sample weight
- The preparation of the standard
- Internal standard technique
- Matrix calibration curve
- The mass used in the test



# Bangkok, Thailand

**ASIA MEDICAL AND AGRICULTURAL  
LABORATORY AND RESEARCH CENTER**



361, 361/1-4 Ladprao Soi  
122, Wangthonglang,  
Bangkok, Thailand 10310





# Certificate ISO 17025

1. Bureau of Laboratory Quality Standards  
Department of Medical Sciences.
2. National Bureau of Agricultural Commodity and Food Standards  
The Ministry of Agriculture and Cooperatives
3. Bureau of Laboratory Accreditation  
Department of Science Service
4. Department of Agriculture
5. Thai Industrial Standards Institute



# Contact us

AMARC Tel : 66 2 9342381-3

- Sales : ext.106,108
- Customer Service : ext. 104, 111
- Fax : 66 2 9340661

Website : [www.amarc.co.th](http://www.amarc.co.th)



ASIA MEDICAL AND AGRICULTURAL LABORATORY AND RESEARCH CENTER

# Thank You

